


# Extraction of Patulin From Apple Juice Using ISOLUTE® Myco prior to LC-MS/MS Analysis

This application note describes a Solid Phase Extraction (SPE) protocol for the extraction of patulin from clear apple juice using the mycotoxin specific ISOLUTE® Myco columns prior to quantitative LC-MS/MS analysis.

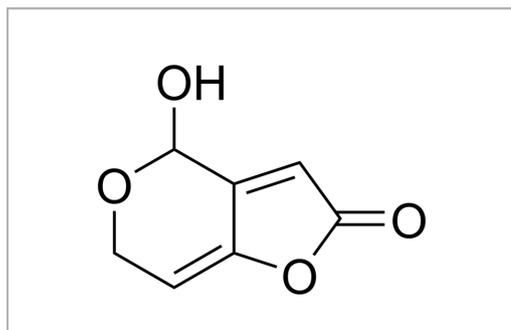

**Figure 1.** Structure of Patulin

## Introduction

Patulin is a mycotoxin produced by *Aspergillum* and *Penicillium* mold species commonly found on rotting apples. Although not a particularly potent toxin, patulin has been shown to be genotoxic and potentially carcinogenic, requiring regulation and analysis in all apple based products. Recommended maximum limits for patulin are set globally at 10 µg kg<sup>-1</sup> in apple juice, 25 µg kg<sup>-1</sup> in solid apple foods and 10 µg kg<sup>-1</sup> for apple based baby food.

This application note achieves high recoveries of patulin from apple juice with RSDs below 10%. Limits of quantitation are 10 µg kg<sup>-1</sup> (calculated from the signal to noise ratio).

ISOLUTE Myco SPE columns provide robust, reliable sample preparation for multiple mycotoxin classes from a wide range of foodstuffs. Using a single, easy to use sample preparation product, along with optimized matrix specific application notes, scientists can prepare diverse food/crop samples for analysis by LC-MS/MS.

## Analytes

Patulin

## Sample Preparation Procedure

<b>Column configuration:</b>	ISOLUTE Myco 60 mg/3 mL (Tablets) part number 150-0006-BG
<b>Sample pre-treatment:</b>	Dilute apple juice 1:1 (v/v) with 10 mM ammonium acetate pH 5. Adjust total volume to pH 5 using 25% ammonium hydroxide (conc) (62.5 µL per mL of apple juice).
<b>Condition:</b>	Condition the column with acetonitrile (2 x 1 mL).
<b>Equilibration:</b>	Equilibrate column with 10 mM ammonium acetate pH 5 (1 mL).
<b>Sample loading:</b>	Load pre-treated sample (1 mL) onto the column.
<b>Interference wash 1:</b>	Wash the column with 10 mM ammonium acetate pH 5 (3 x 1 mL).
<b>Drying:</b>	Dry the column for 5 minutes at maximum pressure, 2 bar/29 psi.
<b>Interference wash 2:</b>	Wash the column with toluene (1 mL).
<b>Drying:</b>	Dry the column for 5 minutes at maximum pressure, 2 bar/29 psi.
<b>Elution</b>	Elute with acetonitrile (1 mL).
<b>Post elution:</b>	The eluate is dried in a stream of air or nitrogen using a SPE Dry (20 to 40 L min <sup>-1</sup> ) or TurboVap LV (15 bar at 30 °C for 40 min). Reconstitute in water (500 µL, HPLC or deionized) prior to analysis.
<b>Note:</b>	This method was developed using the Biotage PRESSURE+ 48 positive pressure manifold, but columns can also be processed using VacMaster sample processing manifolds.

## HPLC Conditions

<b>Instrument:</b>	Waters Alliance 2795
<b>Column</b>	Kinetex phenyl-hexyl 50 mm x 2.1 mm 2.6 µm dp. (Phenomenex inc., Torrance CA)
<b>Mobile phase:</b>	A: Water (HPLC grade) B: Acetonitrile
<b>Flow rate:</b>	0.3 mLmin <sup>-1</sup>
<b>Injection:</b>	10 µL (partial loop) from 20 µL
<b>Gradient:</b>	Initial 15 % B, hold for 1 min Linear ramp to 100 % B in 1 min, hold for 1 min Linear ramp to initial conditions in 0.5 min, hold for 2 min Total run time 4.5 min
<b>Column temp:</b>	Room temperature
<b>Sample temp:</b>	15 °C

## Mass Spectrometry Conditions

<b>Instrument:</b>	Waters Ultima Platinum QQQ
<b>Source:</b>	Electrospray, negative ion mode
<b>Desolvation temp:</b>	350 °C
<b>Quadrupole:</b>	100 °C
<b>Capillary:</b>	3000 kv
<b>Mode:</b>	MRM

**Table 1.** MRM Parameters


Analyte	MRM	Entrance potential	Collision energy (eV)
Patulin (quant ion)	153 > 109	40	8
Patulin (qual ion)	153 > 81	35	10
Hydroxymethylfurfural	125 > 97	40	8


## Results

The extraction method demonstrates high recovery of patulin whilst effectively resolving hydroxymethylfurfural (HMF), which can be a source of chromatographic interference when analysed using less selective analytical methods. Mean analyte recoveries of 101% were achieved for patulin (n=7) with RSDs <10% as shown in table 2. Each chromatogram is shown separately in figure 2 and then overlaid to show actual resolution in figure 3. The limit of quantitation was calculated to be 10 µg kg<sup>-1</sup> based upon an observed signal to noise ratio of 16:1, easily meeting the regulatory limits set for patulin minimum residue limits.

**Table 2.** Typical recoveries of patulin , quant and qual ions (n=7)

	Patulin Quant (153>109) % recovery	Patulin Qual (153>81) % recovery
1	99.60	104.30
2	95.40	98.40
3	97.30	100.00
4	103.60	100.10
5	92.40	91.90
6	104.50	98.20
7	113.60	107.50
Mean	100.91	100.90
% RSD	6.99	3.02

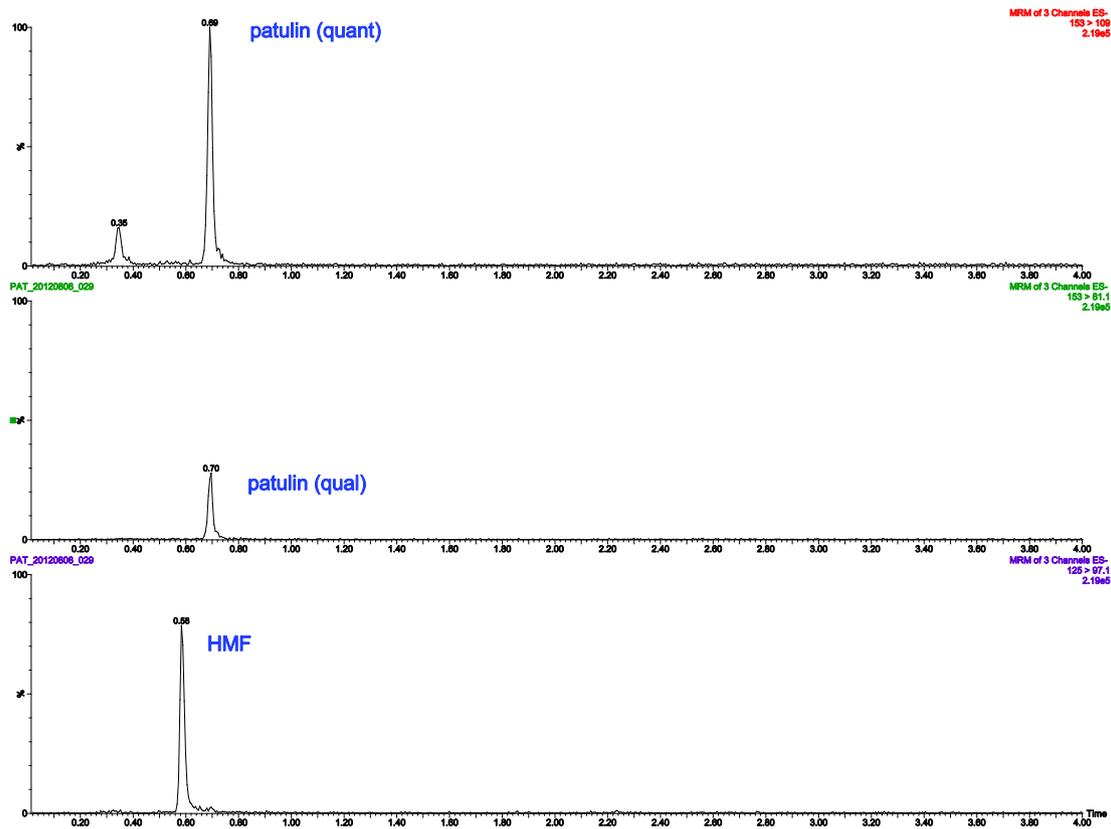
**Figure 2.** Typical chromatogram (10  $\mu\text{g kg}^{-1}$ ) using the ISOLUTE Myco method, showing extracted patulin and the resolved interference analyte HMF

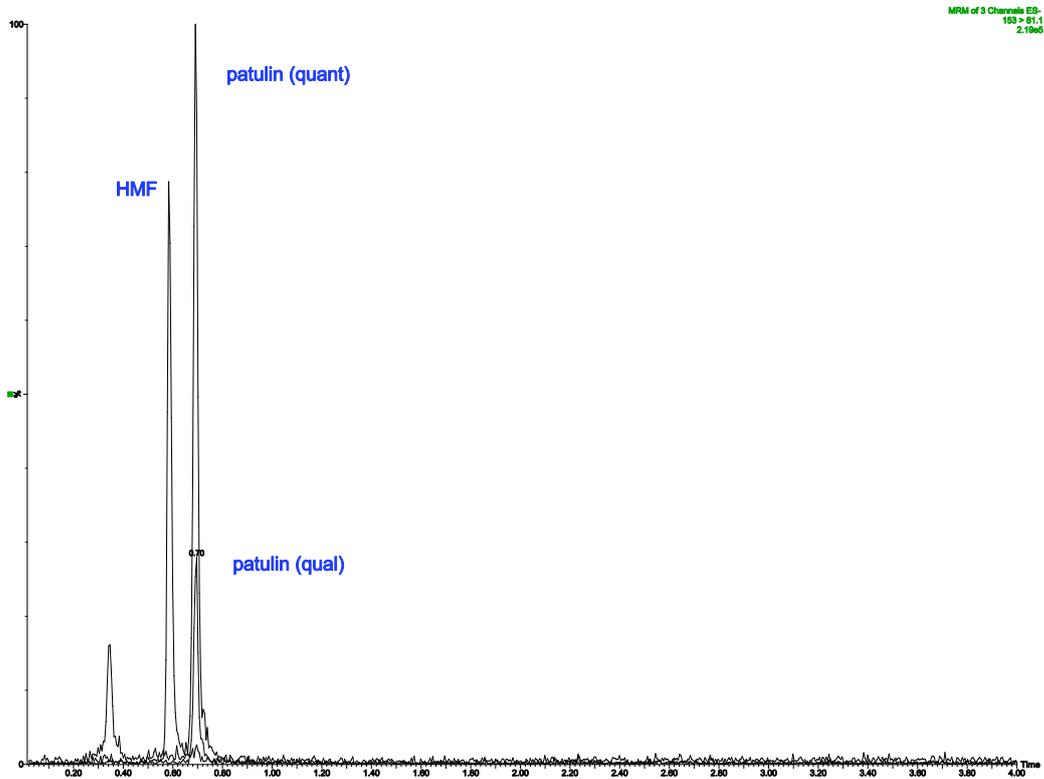

**Figure 3.** Typical overlaid chromatogram as  $10 \mu\text{g kg}^{-1}$  using the ISOLUTE Myco method, showing extracted patulin and the resolved interference analyte HMF

Calibration curves constructed using this method (from  $2\text{-}200 \text{ ng mL}^{-1}$ ), demonstrated excellent linearity with coefficients of determination greater than 0.99 as shown in Figure 4.

Compound name: patulin 153>109  
 Correlation coefficient:  $r = 0.998134$ ,  $r^2 = 0.996271$   
 Calibration curve:  $115.582 * x + -141.87$   
 Response type: External Std, Area  
 Curve type: Linear, Origin: Include, Weighting: Null, Axis trans: None

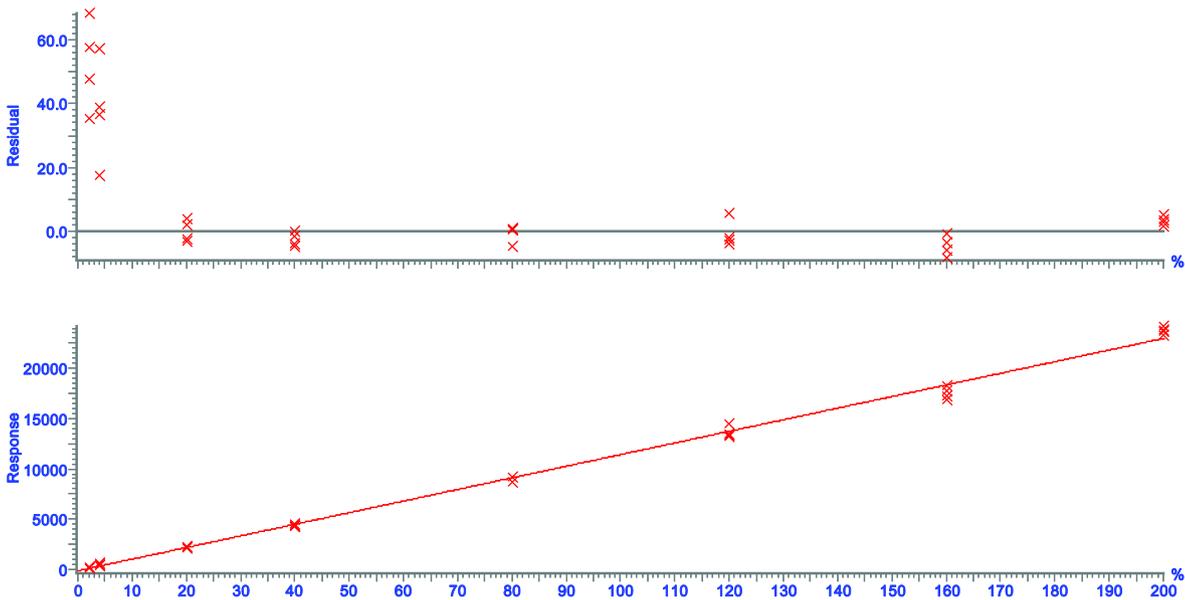

**Figure 4.** Calibration curves constructed using this method from  $2\text{-}200 \text{ ng mL}^{-1}$

## Ordering information

Part Number	Description	Quantity
150-0006-BG	ISOLUTE Myco 60 mg/3 mL column (Tablets)	50
PPM-48	Biotage PRESSURE+ 48 Positive Pressure Manifold 48 Well	1
121-1016	VacMaster-10 Sample Processing Manifold complete with 16 mm collection rack	1
121-2016	VacMaster-20 Sample Processing Manifold complete with 16 mm collection rack	1
C103198	TurboVap LV, 110V	1
C103199	TurboVap LV, 220V	1

For the latest application notes and more information about ISOLUTE® Myco please visit [www.biotage.com/isolutemyco](http://www.biotage.com/isolutemyco) or scan the QR code with your smart phone to go direct.



### EUROPE

Main Office: +46 18 56 5900  
 Toll Free: +800 18 565710  
 Fax: +46 18 59 1922  
 Order Tel: +46 18 56 57 10  
 Order Fax: +46 18 56 57 05  
[order@biotage.com](mailto:order@biotage.com)  
[EU-1-pointsupport@biotage.com](mailto:EU-1-pointsupport@biotage.com)

### NORTH AMERICA

Main Office: +1 704 654 4900  
 Toll Free: +1 800 446 4752  
 Fax: +1 704 654 4917  
 Order Tel: +1 704 654 4900  
 Order Fax: +1 434 296 8217  
[ordermailbox@biotage.com](mailto:ordermailbox@biotage.com)  
[US-1-pointsupport@biotage.com](mailto:US-1-pointsupport@biotage.com)

### JAPAN

Tel: +81 3 5627 3123  
 Fax: +81 3 5627 3121  
[jp\\_order@biotage.com](mailto:jp_order@biotage.com)  
[JP-1-pointsupport@biotage.com](mailto:JP-1-pointsupport@biotage.com)

### CHINA

Tel: +86 21 2898 6655  
 Fax: +86 21 2898 6153  
[cn\\_order@biotage.com](mailto:cn_order@biotage.com)  
[CN-1pointsupport@biotage.com](mailto:CN-1pointsupport@biotage.com)  
[www.biotage.com](http://www.biotage.com)

For regional distributors, products and offers, please visit [www.biotage.com](http://www.biotage.com)