




## Method Development in Solid Phase Extraction using ISOLUTE® SCX and SCX-3 SPE Columns for the Extraction of Aqueous Samples

This technical note includes specifics on the use of ISOLUTE® SCX and SCX-3 for the extraction of cationic analytes from aqueous samples (pages 1-2), ordering information (page 3) and a general discussion on cation exchangers (pages 4-5). For information on extraction of cationic analytes from non-aqueous matrixes, contact Argonaut Technologies.

The ISOLUTE family of cation exchange sorbents are used to extract organic cations (basic compounds capable of exhibiting a positive charge) from both aqueous and non-aqueous matrices. See the appendix for more details about these sorbents

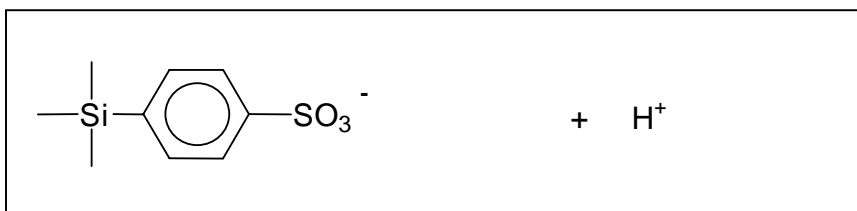

Structure of ISOLUTE SCX sorbent. ISOLUTE SCX-3 is an ethylbenzene sulfonic acid

### In Method Development Using ISOLUTE SCX and SCX-3, the Following Points are Important:

#### Sample Pre-treatment

##### Ionic Strength Control

Ionic strength of the sample should be reduced to <0.05 M by dilution with deionized water or low ionic strength buffer in order to facilitate maximum retention of the analytes. The capacity of a SCX column is approximately 0.35 mM/g of sorbent. The capacity of SCX-3 is approximately 0.6 mM/g of sorbent. The analyte must compete with other cations in the sample for ion exchange sites, so retention of the analyte is reduced when the ionic strength of the sample is high. Dilution will also reduce sample viscosity, to ensure a free-flowing sample. The selectivity of the buffer cation chosen should be considered. Buffers that contain cations of lower selectivity than the analyte facilitate analyte retention. The selectivity of some common cations is as follows (ions on the right will displace those on the left):



ISOLUTE SCX and SCX-3 have a hydrogen counter ion as standard.



## **pH Control**

To ensure that total ionization of the analyte has occurred, the pH of the sample should be adjusted to two pH units below the  $pK_a$  of the analyte [see the two (2) pH unit rule in appendix]. Buffering for pH control should be performed with the lowest strength buffer that will maintain pH, usually 10-20 mM.

## **Column Solvation and Equilibration**

SCX and SCX-3 columns should be solvated with methanol, acetonitrile or THF. For an aqueous matrix both the pH and the ionic strength of the equilibration solvent must be optimized to ensure ionization of the analyte at this stage. Ionic strength should be the same as or very similar to that of the sample, ideally not more than 0.05 M.

## **Sample Loading**

For SCX columns, typical flow rates are 1 mL/min for 1mL columns, 3 mL/min for 3 mL columns and 7 mL/min for 6 mL columns. The ion exchange process will not occur efficiently if the flow rate is too high.

## **Interference Elution**

For SCX columns, ionic strength and pH control should be maintained to prevent analyte loss. The same buffer as the equilibration buffer is often suitable. An initial wash with 0.01 M acid followed by acidified methanol or acetonitrile (up to 30%) in water is often suitable for removing lipophilic interferences. It should be noted that the  $pK_a$  of compounds can be altered in a solution containing organic solvent, so care should be taken to avoid losses of analytes in this way.

## **Analyte Elution**

### **Displacement of the Analyte by Mass Action**

To minimize elution volumes, the elution solvent must overcome both the primary ionic retention mechanism, and the secondary non-polar interactions. Unless the analyte is a very polar, water soluble compound, then some solvent component is essential. Buffers with an ionic strength of  $>0.1$  M containing 25-50% organic solvent (e.g. methanol) are suitable. Methanol containing a soluble salt such as ammonium acetate (0.1 M) is also a suitable elution solvent.

If a non-aqueous elution solvent is required, for example if the eluent is to be injected directly into a GC, evaporated to give a higher concentration of analyte, or derivatized prior to analysis, then organic solvents, modified with a volatile base such as tetramethyl ammonium hydroxide (2-5% v/v) are suitable.

### **Neutralization of the Charge on the Analyte (Weak Cations Only)**

Weak cations can be eluted using a buffer/solvent mixture or solvent adjusted to two (2) pH units above the  $pK_a$  of the analyte.

In order to minimize elution volumes, ISOLUTE SCX and SCX-3 SPE columns are available in a range of sizes, starting at 25 mg (for elution volumes of less than 100  $\mu$ l), up to 10 g.

## ISOLUTE SCX and SCX-3 Product Ordering Information

Product Description	Columns / Box	ISOLUTE SCX Part Number	ISOLUTE SCX-3 Part Number
25 mg/1 mL	100	530-0002-A	533-0002-A
50 mg/1 mL	100	530-0005-A	533-0005-A
50 mg/10 mL	50	530-0005-G	533-0005-G
100 mg/1 mL	100	530-0010-A	533-0010-A
100 mg/3 mL	50	530-0010-B	533-0010-B
100 mg/10 mL	50	530-0010-G	533-0010-G
200 mg/1 mL	100	530-0020-A	533-0020-A
200 mg/3 mL	50	530-0020-B	533-0020-B
200 mg/10 mL	50	530-0020-H	533-0020-H
500 mg/3 mL	50	530-0050-B	533-0050-B
500 mg/6 mL	30	530-0050-C	533-0050-C
500 mg/10mL	50	530-0050-H	533-0050-H
1 g/3 mL	50	530-0100-B	533-0100-B
1 g/6 mL	30	530-0100-C	533-0100-C
2 g/15 mL	20	530-0200-D	533-0200-D
5 g/25 mL	20	530-0500-E	533-0500-E
10 g/70 mL	16	530-1000-F	533-1000-F

These sorbents are also available in the high throughput 96-well SPE plates, ISOLUTE-96 and ISOLUTE Array. Please contact Biotage for further information.

## APPENDIX

### ISOLUTE Cation Exchange Sorbents: SCX, SCX-2 (PRS), SCX-3 and CBA


The ISOLUTE family of cation exchange sorbents are used to extract organic cations (basic compounds capable of exhibiting a positive charge) from both aqueous and non-aqueous matrixes. Although extraction is by the same mechanism, each sorbent has properties that influence the way they are used.

Cation exchange SPE can be accomplished by strong (low  $pK_a$ ) and weak (higher  $pK_a$ ) ion exchangers. Both **SCX** and **SCX-3** (benzenesulfonic acid and ethylbenzene sulfonic acid phases respectively— see structure on page 1) and **SCX-2 (PRS)** (a propylsulfonic acid phase) are strong cation exchangers. They maintain a permanent negative charge over the whole pH range (pH 1-14). **SCX and SCX-3 have significant non-polar character due to the aromatic ring, so secondary non-polar interactions with analytes are present. This can enhance recoveries, but a proportion of organic solvent in the elution solvent is necessary to overcome secondary interactions and elute analytes efficiently.** **SCX-2** has very little non-polar character, and is the strong cation exchanger of choice if the elution solvent must be totally aqueous. The additional strong secondary interaction of the ISOLUTE **SCX-3** is particularly useful if the sample matrix is high or variable in ionic strength.

**CBA** (a carboxy propyl phase) is a weak cation exchanger, with a  $pK_a$  of 4.8. It is used for the extraction of cations that exhibit a positive charge at pH 6.8 or higher. The charge on the sorbent is neutralized at a pH of 2.8 or less. This can be useful for the extraction of analytes with a permanent positive charge, such as quaternary amines, which cannot be neutralized by pH control.

### Retention and Elution Characteristics of ISOLUTE SCX and SCX-3 Strong Cation Exchange Sorbents

Retention and elution using ISOLUTE SCX are illustrated on page 5. The same mechanisms apply to the ISOLUTE SCX-3 sorbent (not shown).

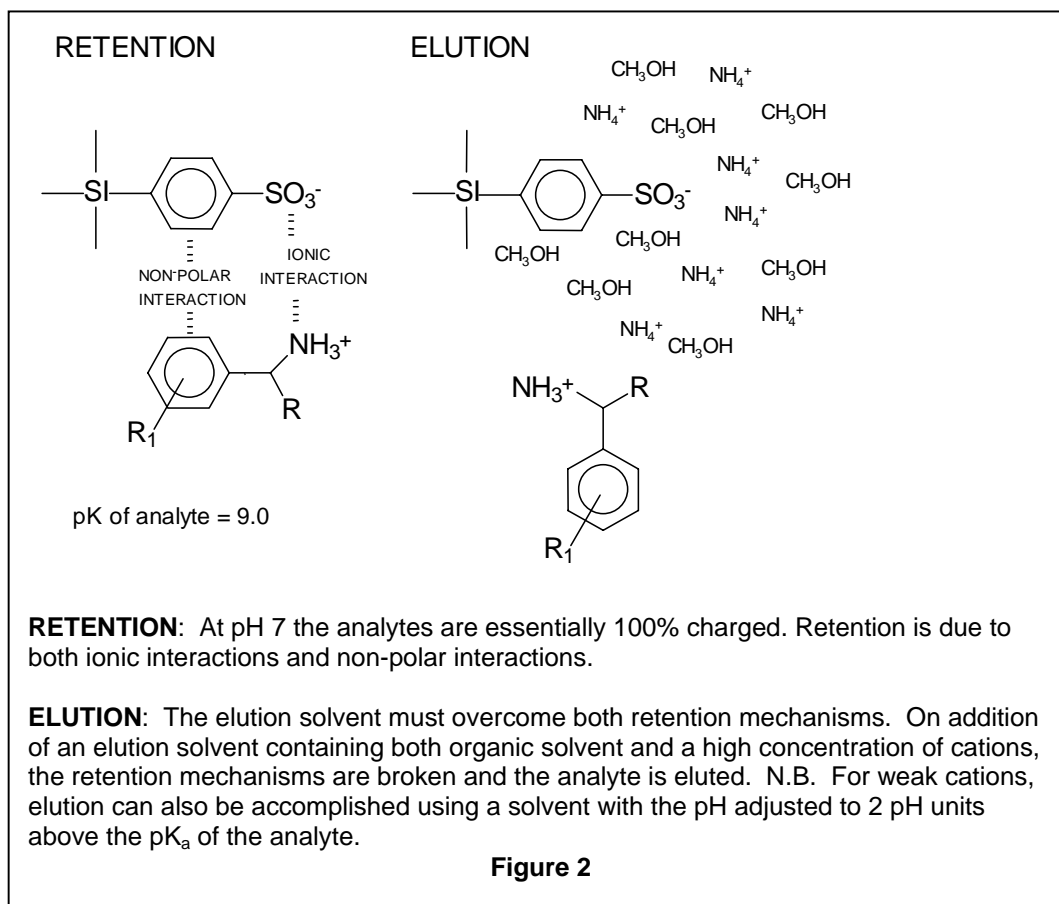

*Retention and elution characteristics of ISOLUTE SCX and SCX-3 cation exchange sorbents*

## The Two (2) pH Unit Rule

The pK<sub>a</sub> of a molecular functional group is defined as the pH at which 50% of this group in solution are charged, and 50% are uncharged. Each pH unit change affects the percentage of charged or uncharged groups by a factor of 10, so it is sensible to perform extractions at a pH at least 2 pH units from the pK<sub>a</sub> value, to ensure that 99.5% of the functional groups are in the desired state.

e.g. Effect of pH on the dissociation of a weak acid with a pK<sub>a</sub> value of 4.0.

pH	% free acid (uncharged)	% dissociated (charged)
4.0	50	50
5.0	5.0	95
6.0	0.5	99.5

e.g. Effect of pH on the dissociation of the conjugate acid of a weak base with a pK<sub>a</sub> value of 9.0

pH	% free base (uncharged)	% dissociated (charged)
9.0	50	50
8.0	5.0	95
7.0	0.5	99.5

**TN106 rev1.3**

ISOLUTE is a registered trademark of a Biotage

©2004 Biotage. All rights reserved.



**United States and Canada**  
Tel: + 1 434 979 2319  
Toll-Free: + 1 800 446 4752  
ordermailbox@biotage.com

**United Kingdom, EIRE**  
Biotage  
Tel: + 44 1443 811811  
eurosales@eu.biotage.com

**Sweden**  
Biotage  
Tel: + 46 18 56 59 00  
order@eu.biotage.com

**Japan**  
Tel: + 81 422 281233  
order.biotage.co.jp

---